


Appendix 34.3: PVDOMICS OMICS HEALTHY CONTROLS Blood and Urine Collection 1: Processing, Aliquoting, Recording and Storing of Biospecimens

Processing needs to start within 1 hour of collection

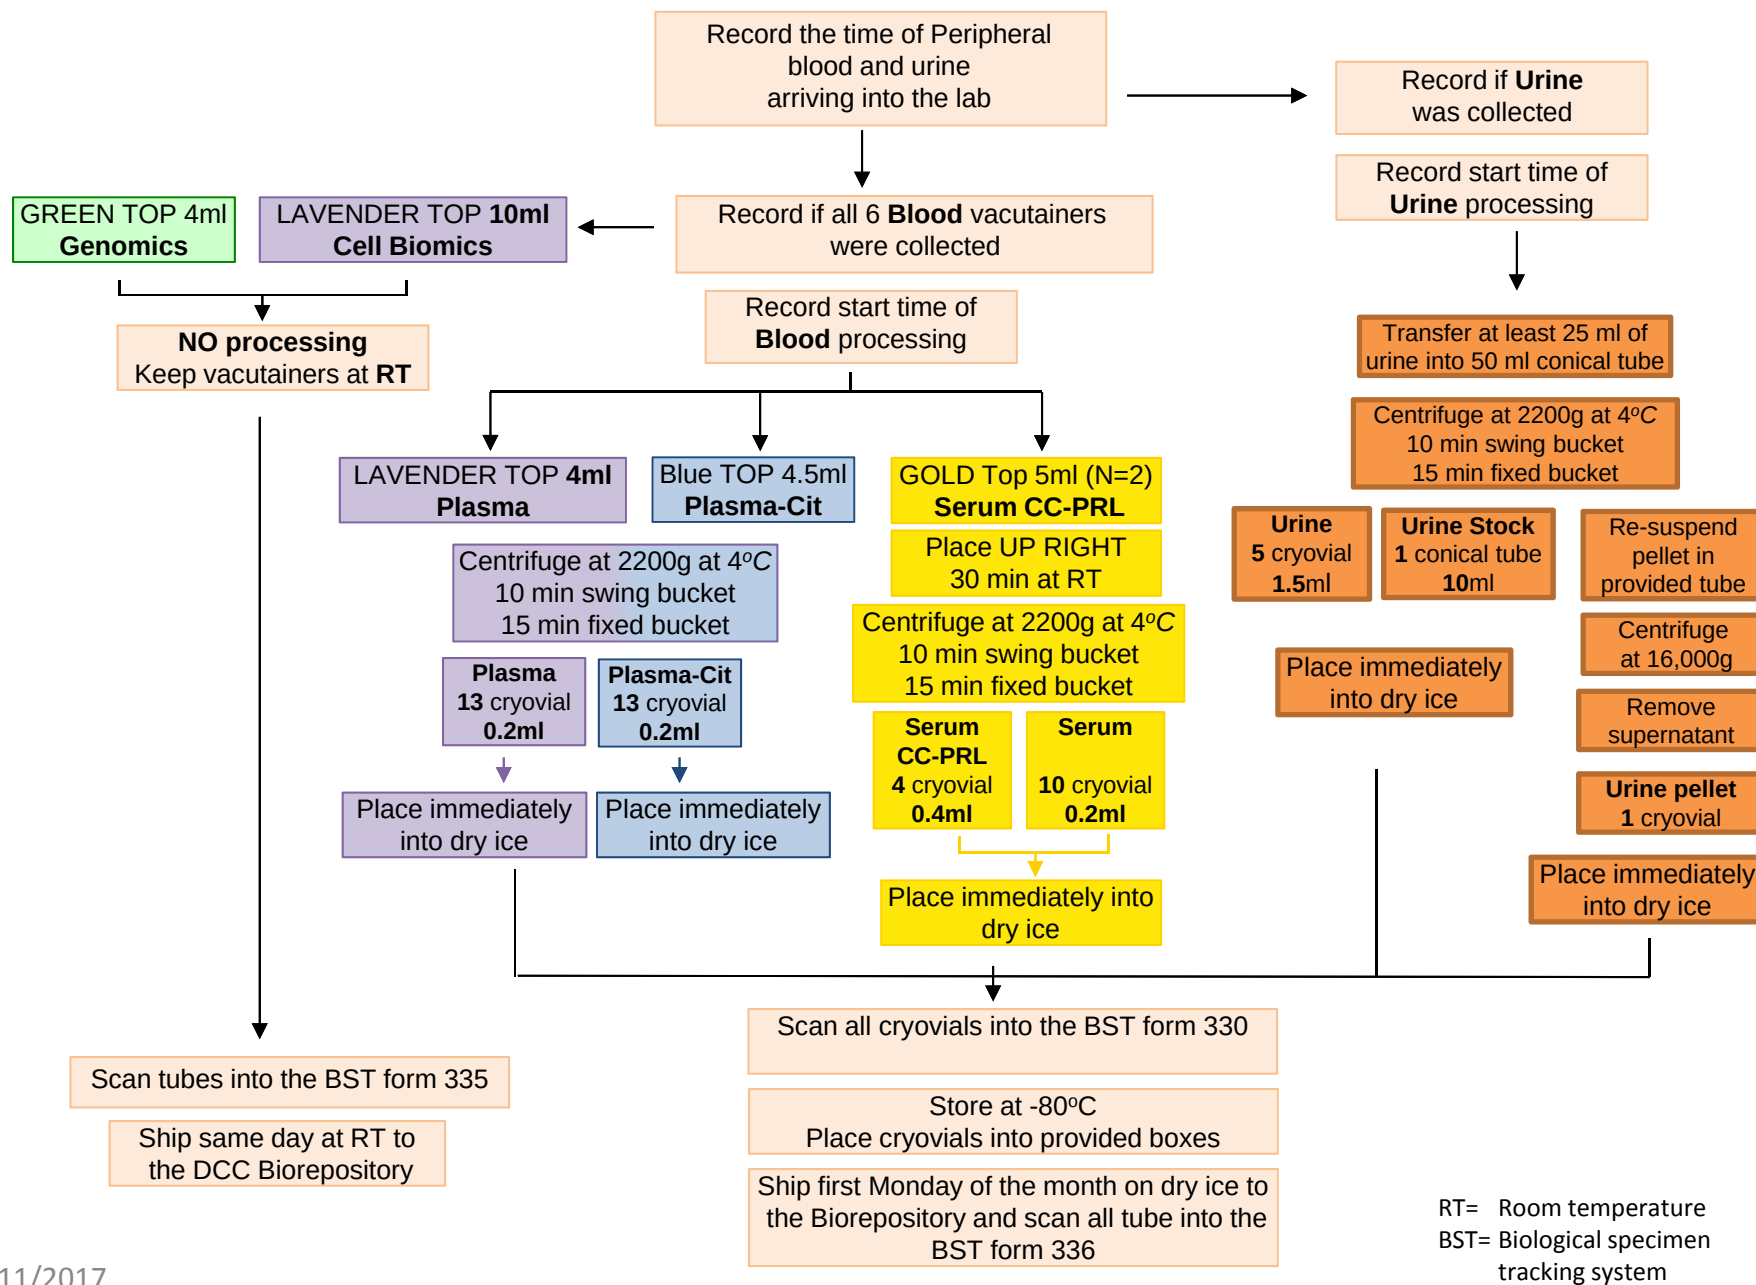

Appendix 34.3: PVDOMICS OMICS Blood Collection 2 HEALTHY CONTROLS:

Processing, Aliquoting, Recording and Storing of Biospecimens

Processing needs to start within 1 hour of collection

Order of processing:

1. Place the Gold top and Red tops up right
2. Centrifuge the 5 Purple tops
3. Cryovial Purple tops
4. Centrifuge Gold top
5. Cryovial Gold top

